

Fig. 1

Schematic view of equipment; not to scale




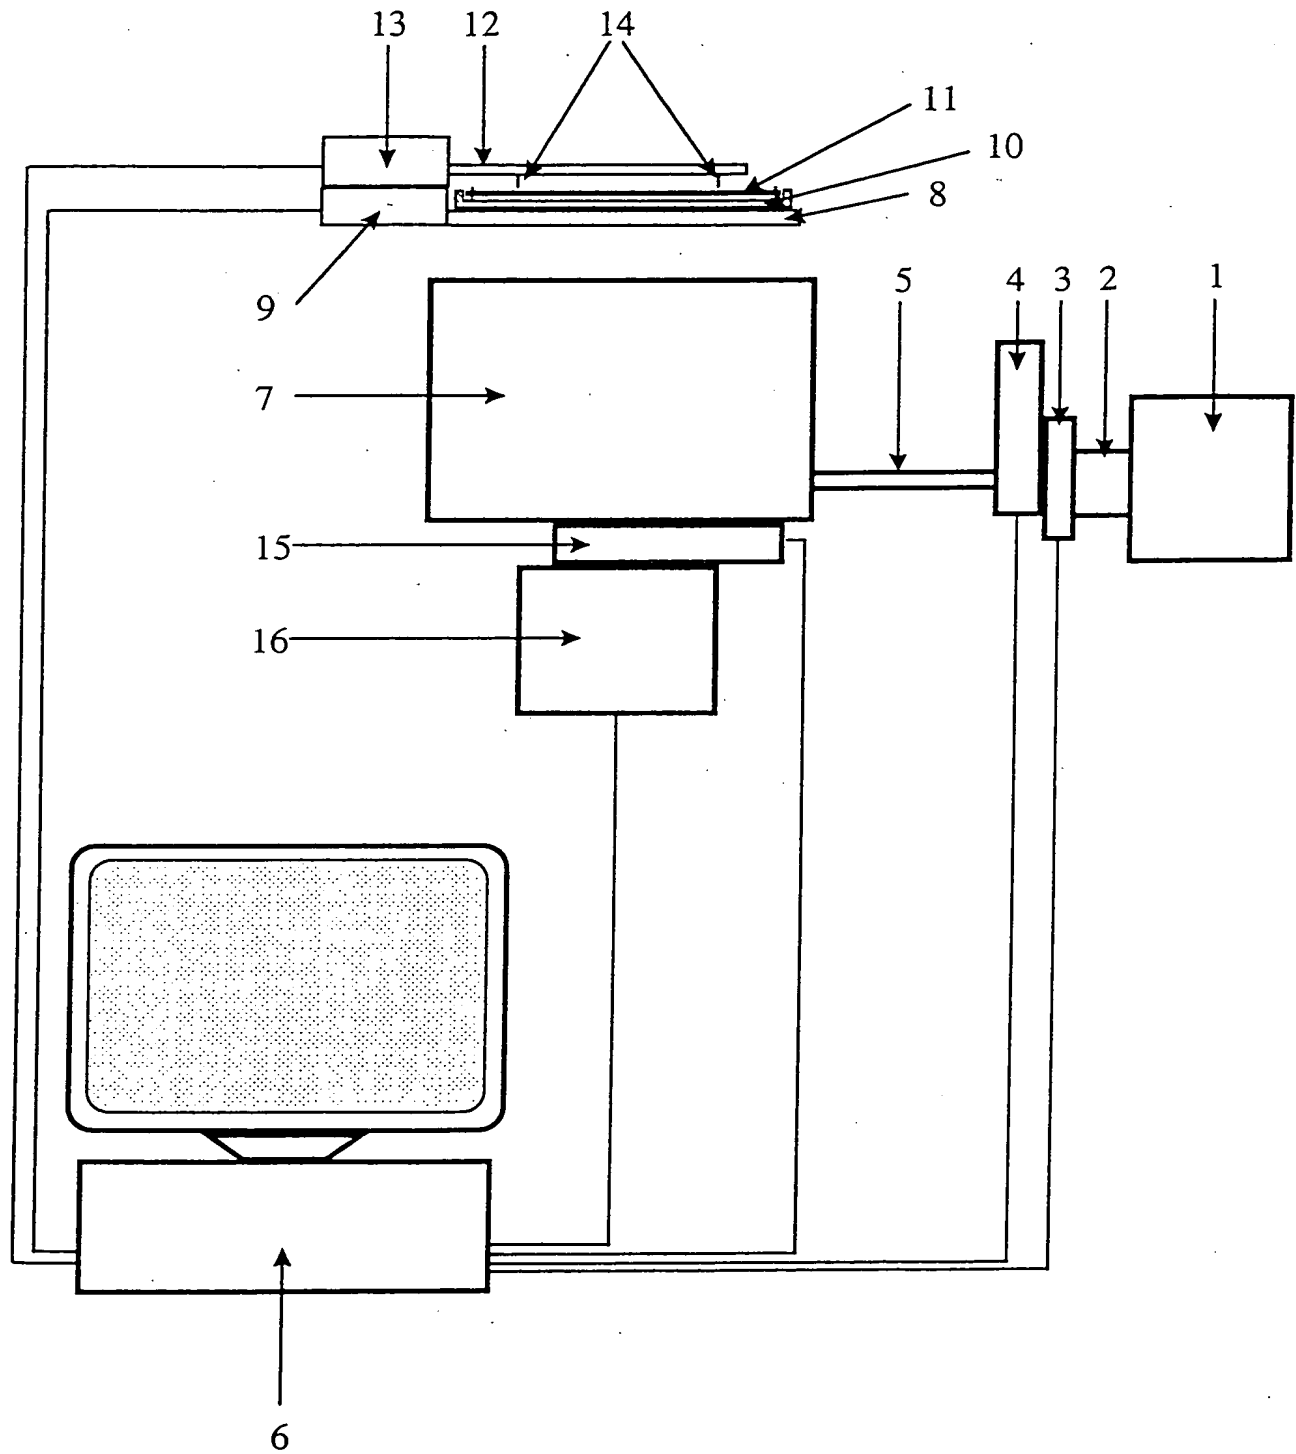


Fig. 2

Side views of test stage; not to scale

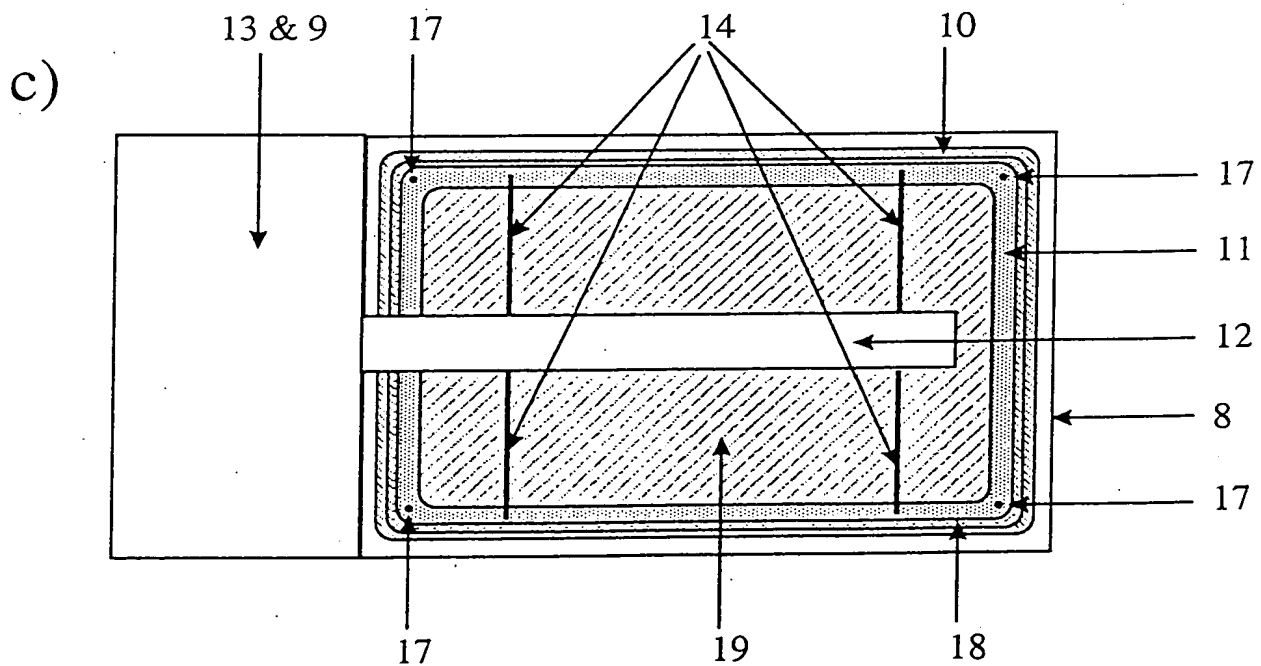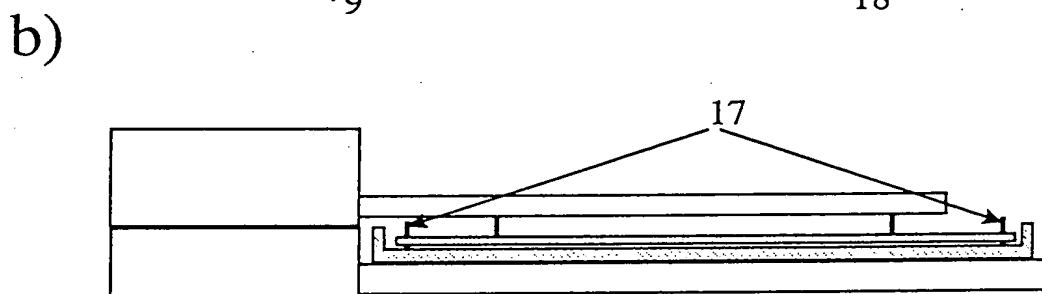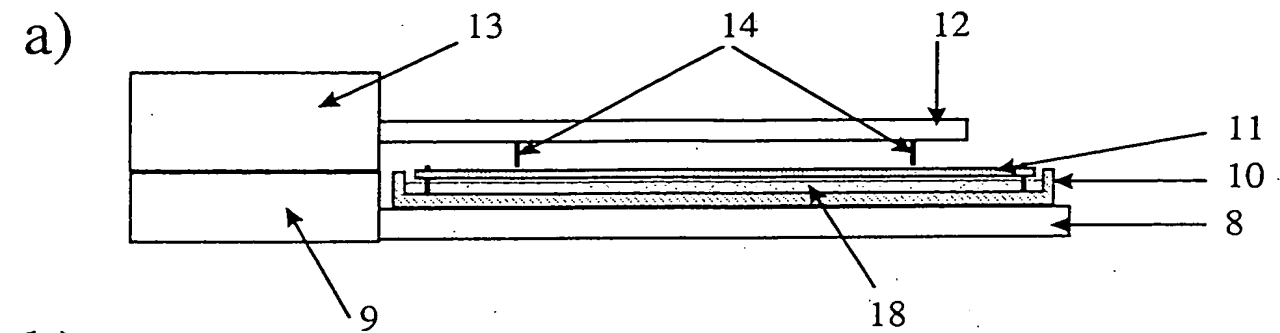

Top view of test stage; not to scale

**3-D sectional representations of portions of
the test-array/detector layers: not to scale**

Fig. 3

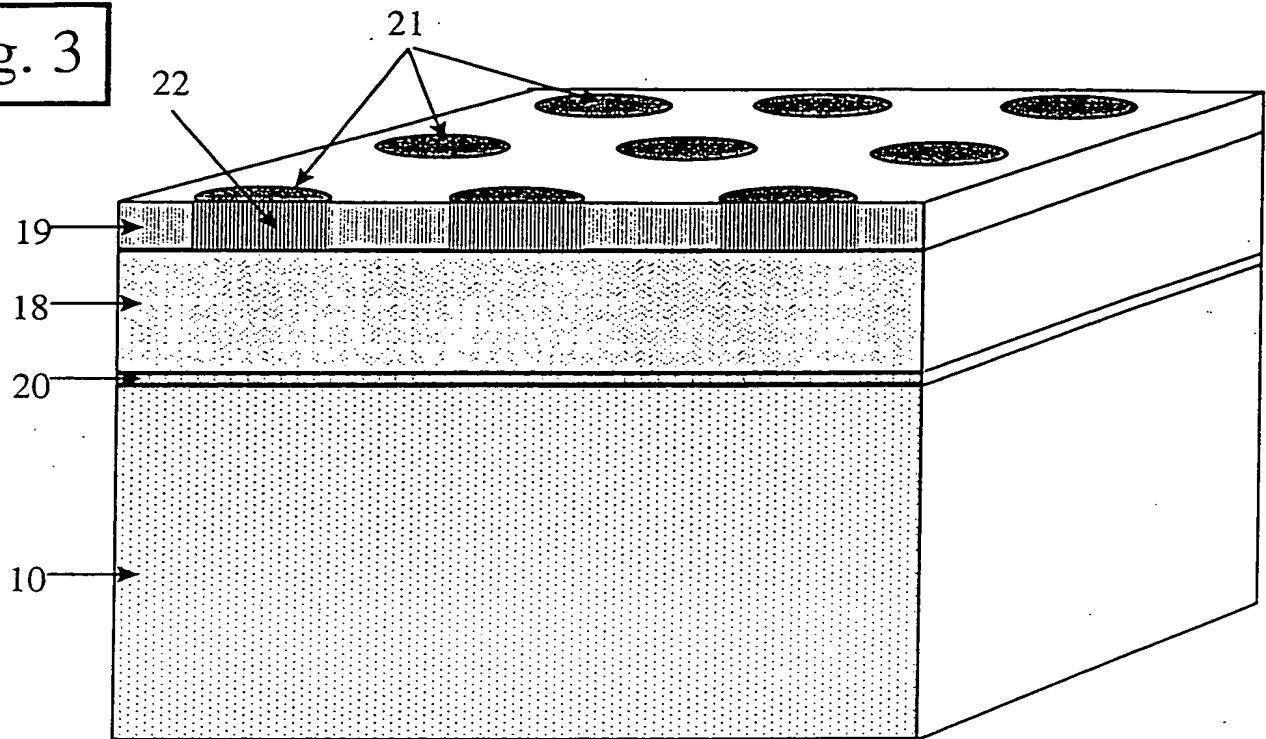


Fig. 4



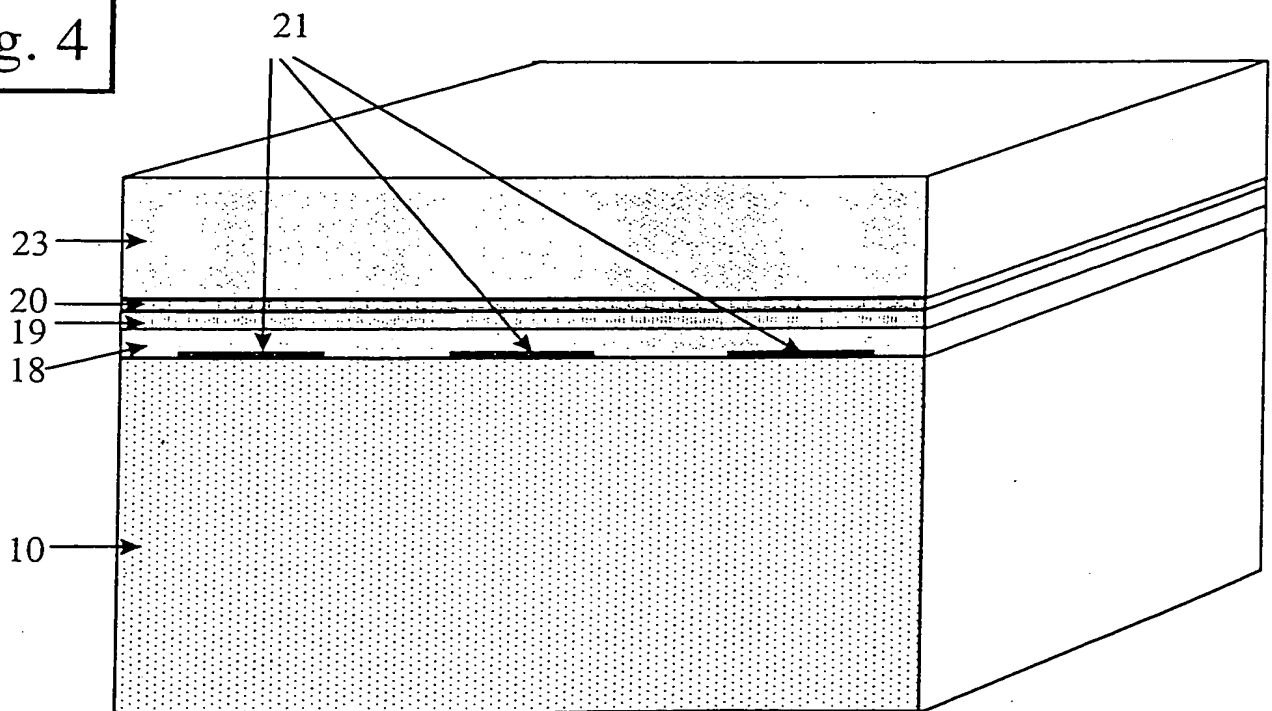


Fig. 5


a)

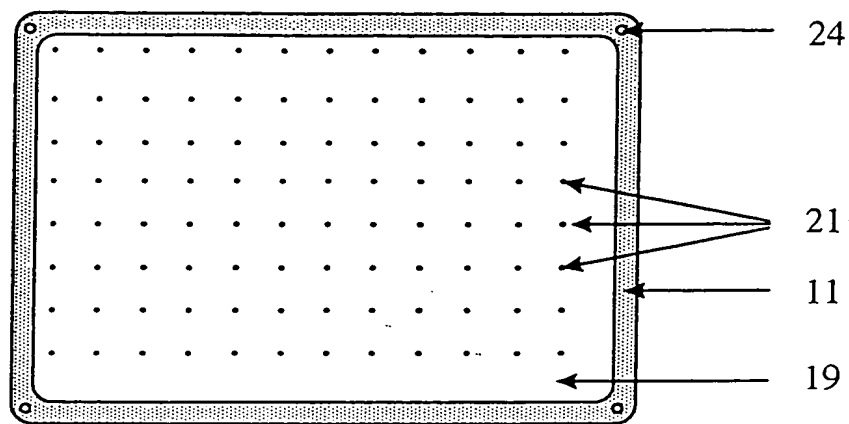

b)

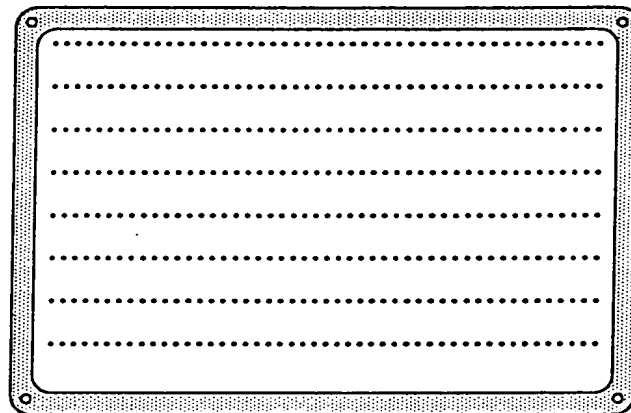

c)

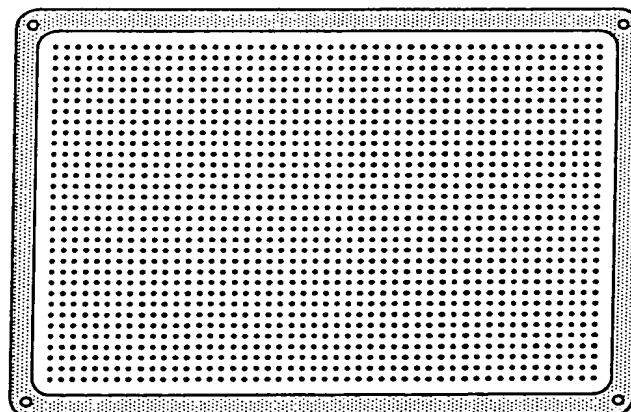

BEST AVAILABLE COPY

Carbamylcholine Response
(1 mM, five spots)

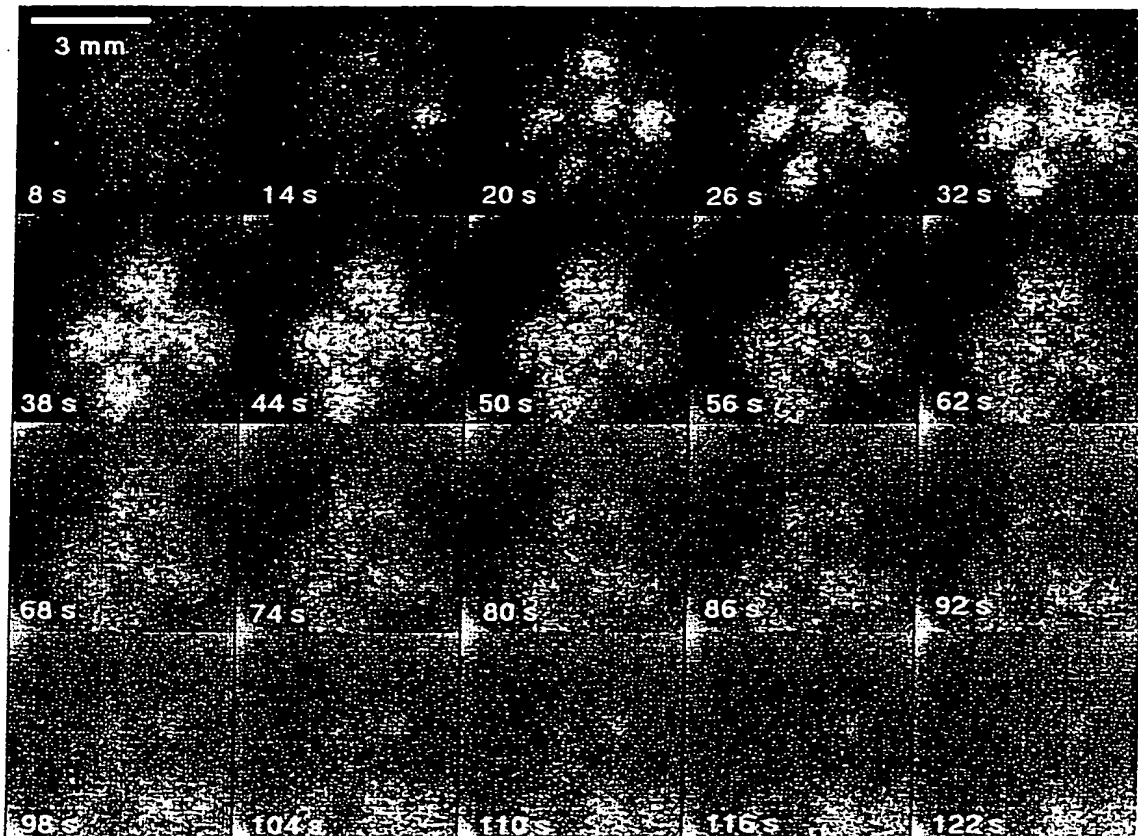


Figure 6

Carbamylcholine Response

(1 mM, five spots)

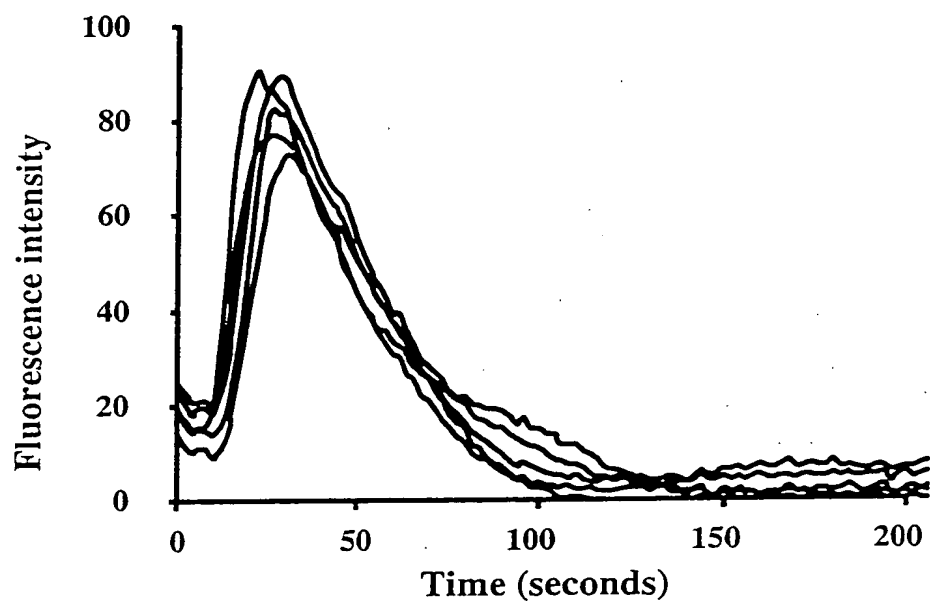


Figure 7

BEST AVAILABLE COPY

FCCP Response
(50 μ M, 5 x 5 grid of spots)

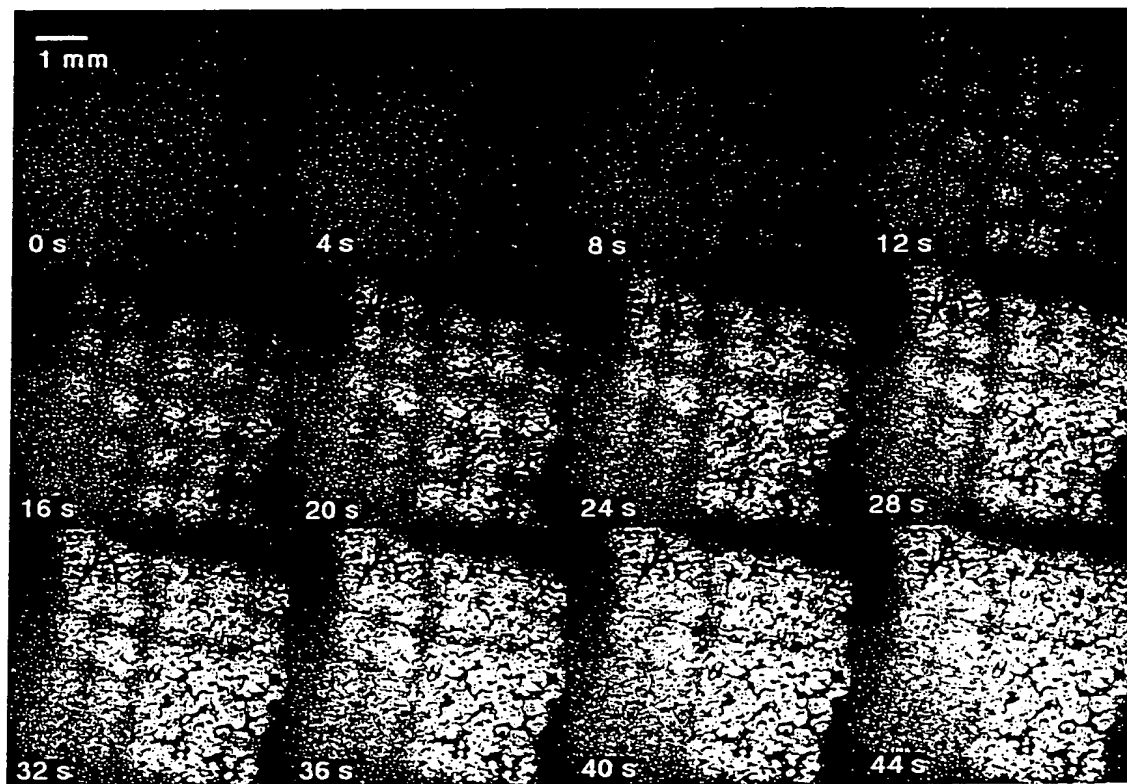


Figure 8

FCCP Response
(50 μ M, five central spots)

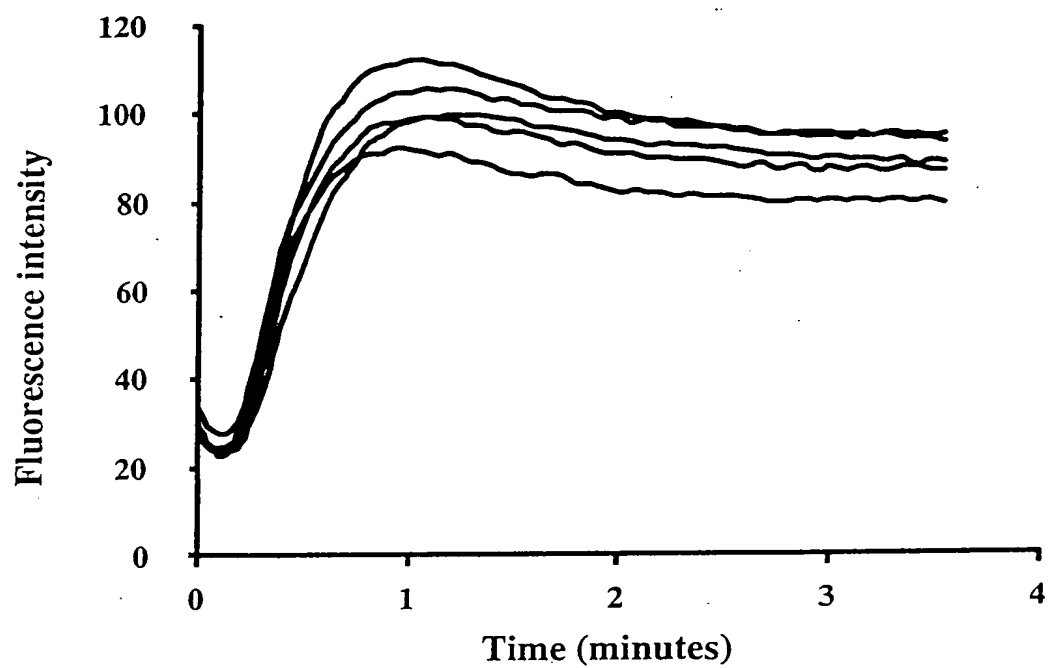


Figure 9

BEST AVAILABLE COPY

FCCP Dose-response
(50, 5, 0.5, 0.05 and 0.005 μ M, 5 x 5 grid)

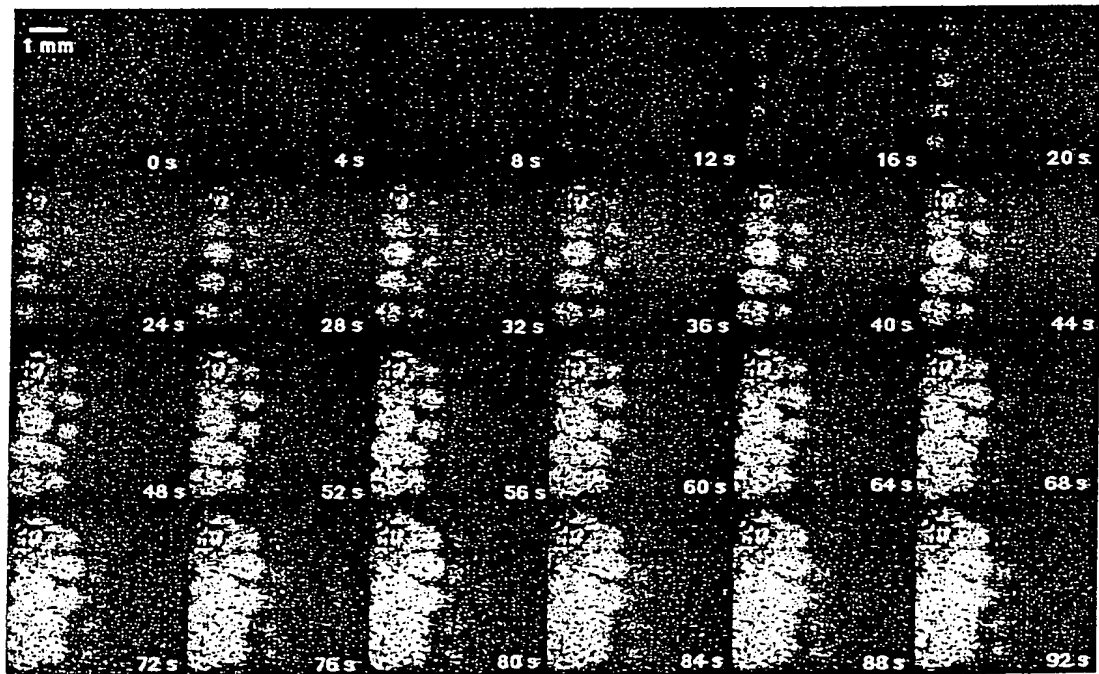


Figure 10

FCCP Dose-response
(50, 5, 0.5, 0.05 and 0.005 μM)

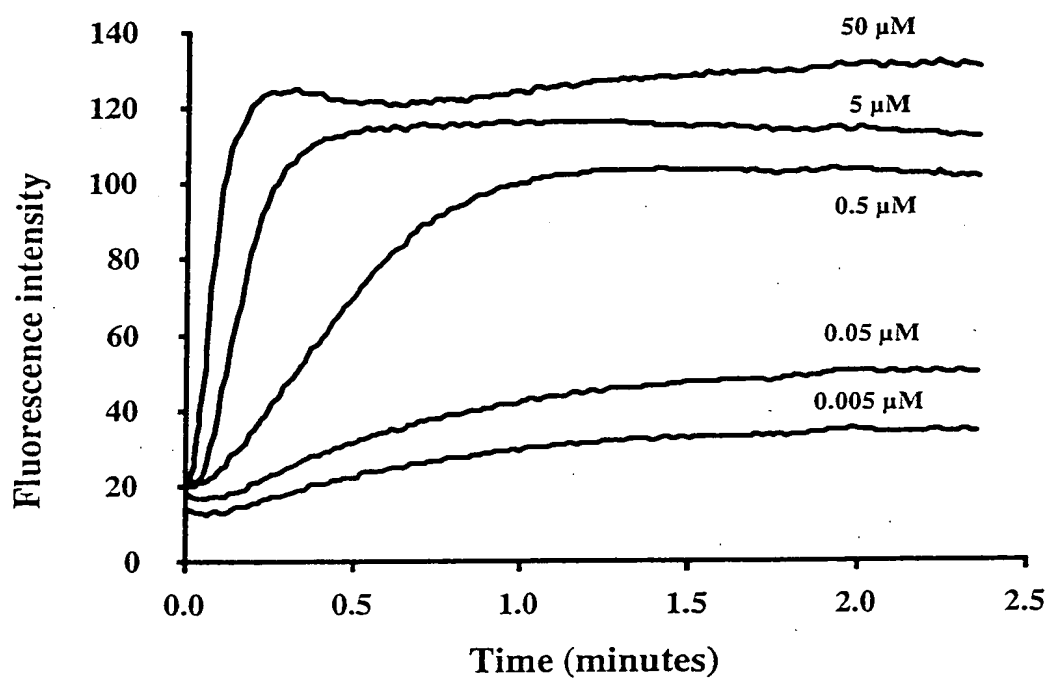


Figure 11

Ionomycin and Thapsigargin responses

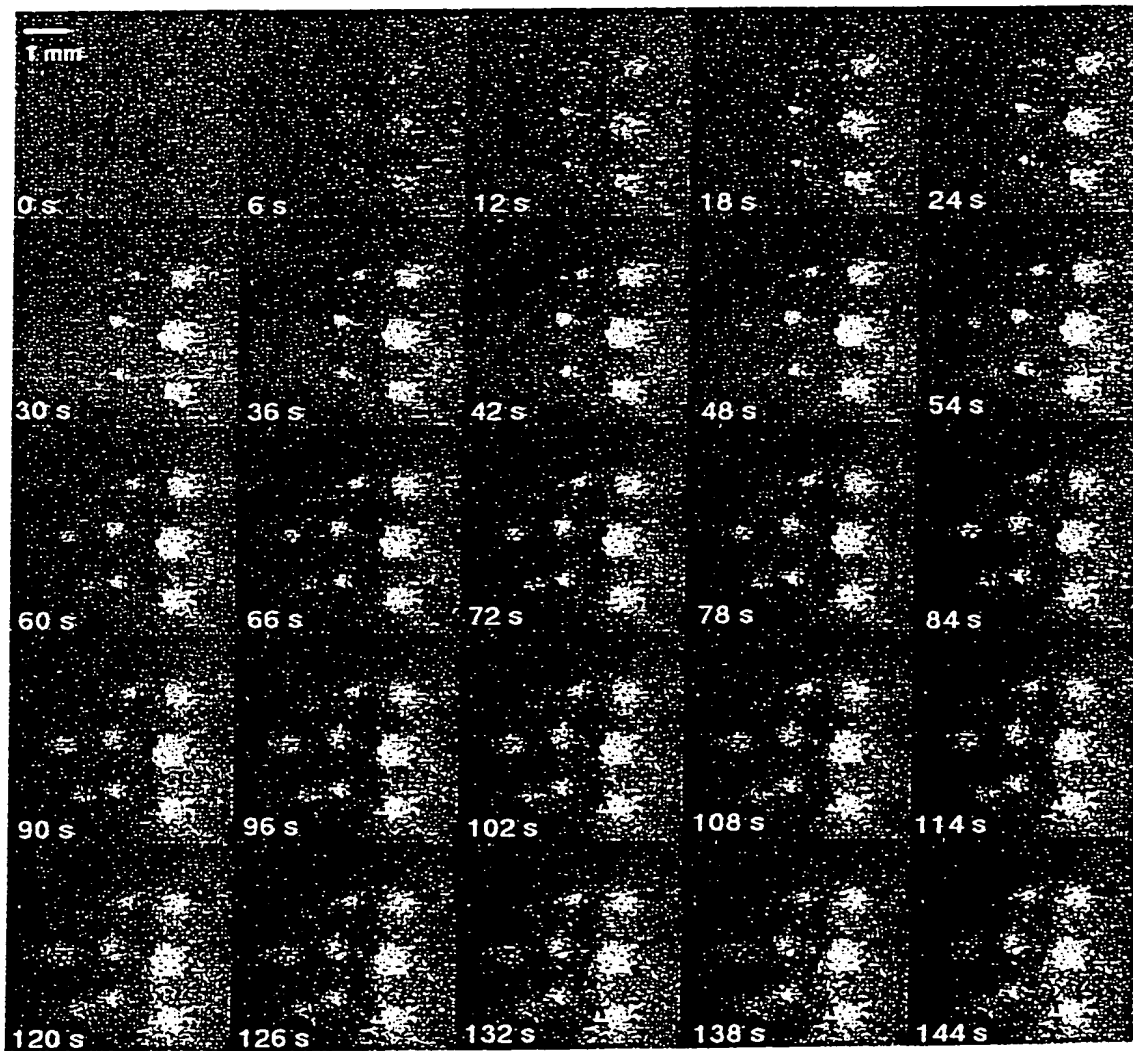


Figure 12

Ionomycin and Thapsigargin responses (mean of two to three responses)

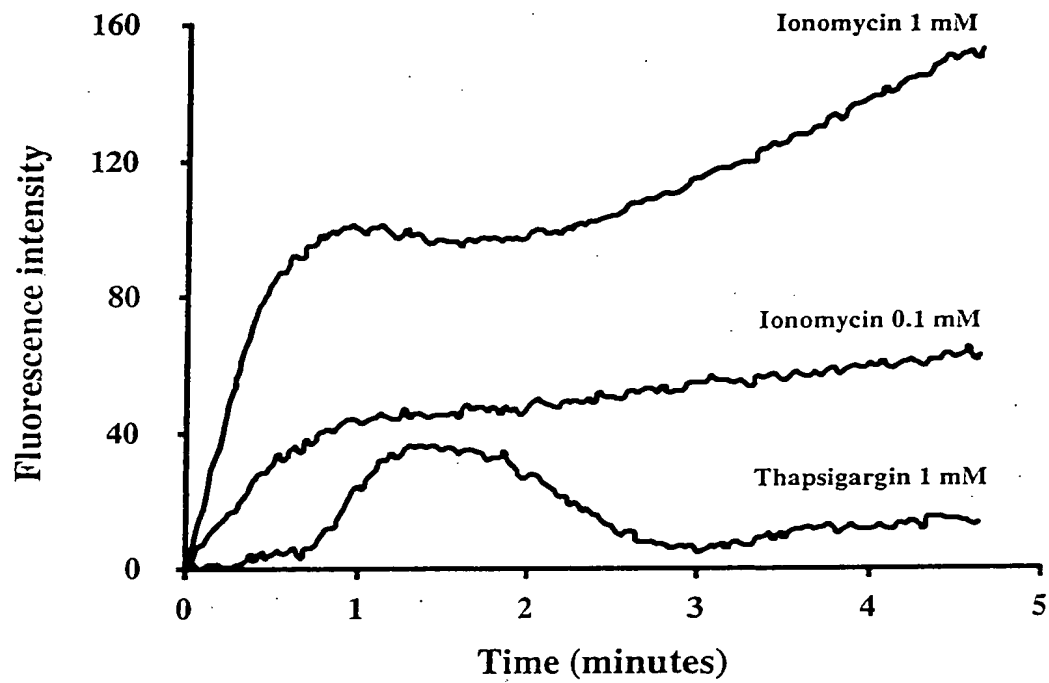


Figure 13